

Test Report

Start Time: 02/03/16 15:23:02 End Time: 12/03/16 14:48:02 Sampling Rate: 5mins Samples: 2874

Air pressure High Alarm: 109.7 kPa LOW Alarm: 70.0 kPa


Temperature High Alarm: 65.6 C Low Alarm: -17.8 C

Relative Humidity High Alarm: 90.0 %RH Low Alarm: 1.0 %RH

Air pressure MAX: 102.82 kPa @17:58:02 11/03/16 MIN: 81.54 kPa @03:48:02 07/03/16 AVG: 98.83 kPa

Temperature MAX: 28.4 C @14:23:02 12/03/16 MIN: 12.4 C @02:33:02 09/03/16 AVG: 20.4 C

Relative Humidity MAX: 54.1 %RH @01:28:02 08/03/16 MIN: 13.4 %RH @13:03:02 03/03/16 AVG: 32.4 %RH

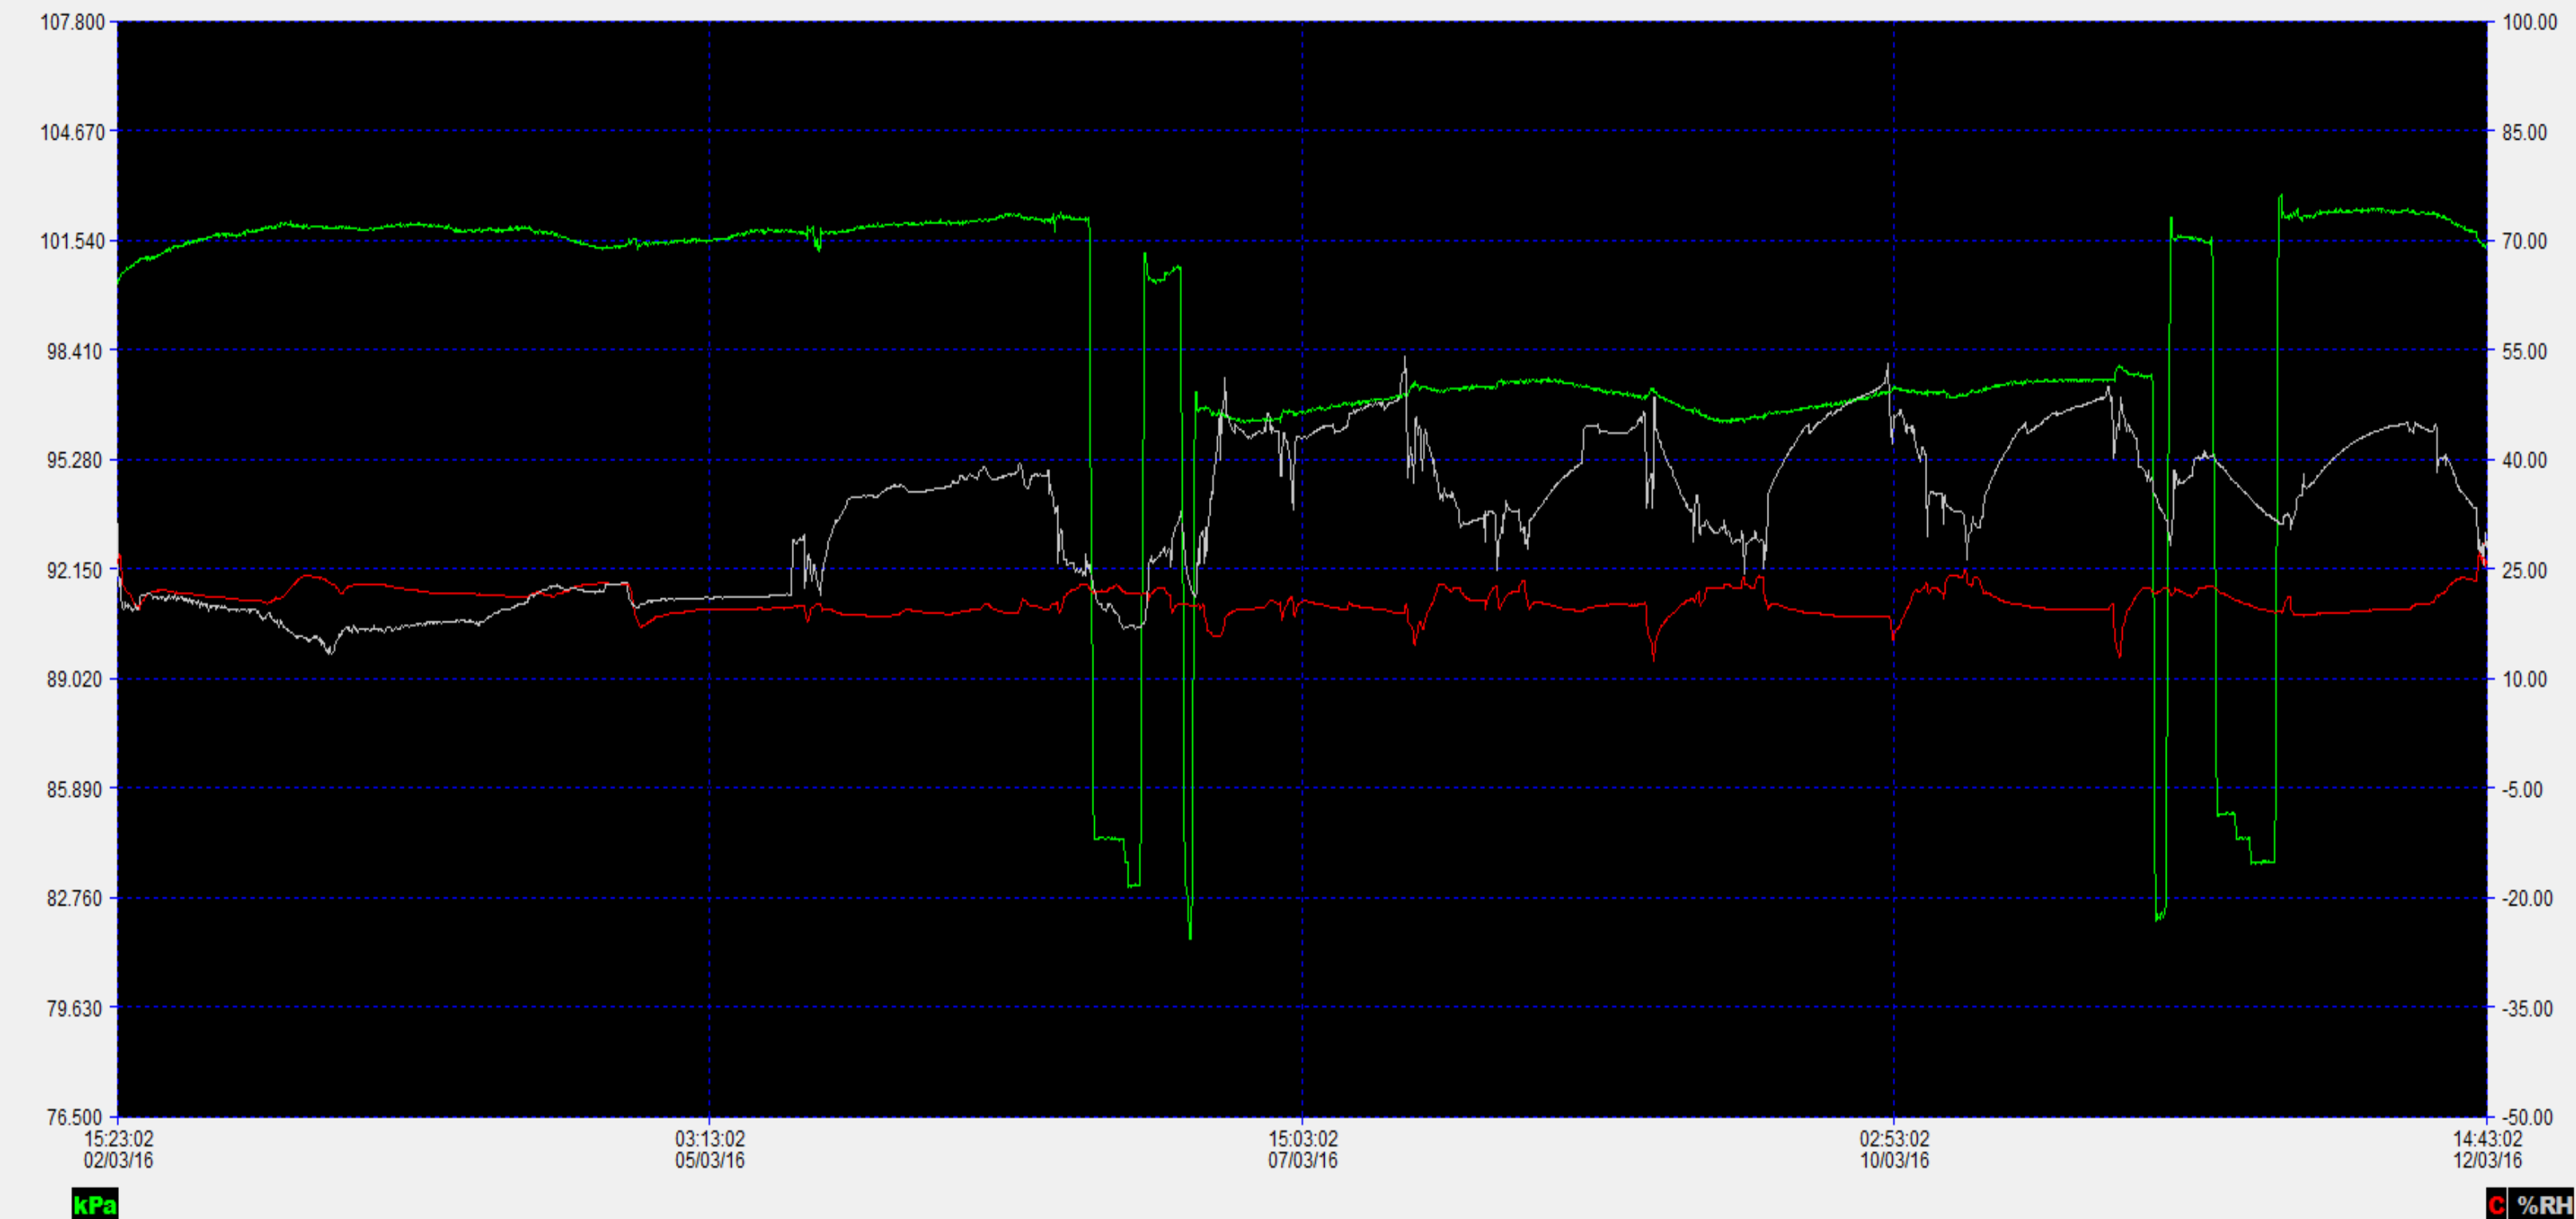

Actual Measurement Time:04/03/16 05:58:02 Point No.:464 Air Pressure:101.87 kPa Temperature:21.3 C Relative Humidity:19.1 %RH